

Comparative Investigation of Reagent Systems (Powder Pack / Pillow) for Free and Total Chlorine from Aqualytic and Hach*

Contents	Page
Introduction and purpose	2
Methods, reagents and equipment employed	2
Part I Calibration with potassium iodate	4
I.1 Results using Aqualytic reagents	4
I.2 Results using HACH reagents	5
I.3 Diagrammatic presentation of results	7
Part II Precision measurements	8
Part III Calibration with potassium permanganate	10
Bibliography	12
Appendix	13

* HACH is a registered trademark of the HACH Company, Loveland, Colorado, USA.

INTRODUCTION AND PURPOSE

In solutions which are slightly acidic in nature (with a pH value of 6.2 to 6.5) N.N-diethyl-1.4-phenylendiamine (DPD) is oxidized with free chlorine, with a red coloured product being produced. Combined chlorine also produces this coloured product in the presence of iodide ions, (total chlorine determination).

Chlorine concentration is measured either by visual colour comparison or by photometry (colorimetry).

The purpose of this present investigation was to compare the powder reagents produced by Messrs. HACH with those of Messrs. Tintometer GmbH (the product name being Aqualytic®) and to demonstrate that the Aqualytic powder packs :

- VARIO CHLORINE FREE - DPD
- VARIO CHLORINE TOTAL - DPD

correspond with HACH "powder pillows" and give the same results when used in association with HACH photometers. The investigation was carried out at the request of Tintometer GmbH.

METHODS, REAGENTS AND EQUIPMENT EMPLOYED

1. Methods

1.1 Measurements according to EN ISO 7393 :

The measurements were carried out in accordance with EN ISO 7393-2 [1]. In deviation from this document, all diluted standards were brought to 100 ml by adding 0.3 ml of a 10% solution of potassium iodide in water¹.

1.2 Measurements obtained with powder reagents :

Measurements were carried out in accordance with the manufacturers' instructions.

1.3 Measurements obtained with potassium permanganate :

Measurements were carried out in accordance with EN ISO 7393-2. The potassium iodate standard was replaced by potassium permanganate standards. Here again, all diluted standards were brought to 100 ml by adding 0.3 ml of a 10% solution of potassium iodide in water¹.

2. Reagents

2.1 Potassium iodate standard solution :

¹The concentration of potassium iodide was inadequate, particularly for very dilute standard solutions .

INSTITUT FRESENIUS

This solution was prepared by weighing 1.006 g of potassium iodate (from Merck) into one litre of water.

2.2 Potassium permanganate standard solution :

This solution was produced by diluting a standard solution (Titrisol from Merck).

2.3 DPD was obtained from Aldrich

2.4 All other reagents were obtained from Merck.

2.5 Powder reagents :

2.5.1 Free chlorine

	<u>Batch Nos.</u>
Aqualytic	204B
Hach	A2256

2.5.2 Total chlorine

Aqualytic	203A
Hach	B2242

2.6 Distilled water was used, without further treatment, to produce the solutions.

3. Equipment

1. Spectrophotometer :

The Spectrophotometer used was a "PERKIN-ELMER, Lambda 2, UV/VIS", with a wavelength of 510 nm, using 1 cm quartz cuvettes.

2. Hach photometer, "DR/890 Colorimeter", with Hach round cuvettes.

I Calibration with potassium iodate

Calibration checks were carried out with powder reagents from Aqualytic and Hach for free and total chlorine. The standards used were potassium iodate solutions according to EN ISO 7393-2: 2000. Measurements were made with a spectrophotometer from Perkin Elmer (1 cm quartz cuvette). For comparison, calibration was also carried out using the method set out in EN ISO 7393-2: 2000.

INSTITUT FRESENIUS

I.1 Measurement results obtained with Aqualytic reagents and their statistical evaluation

Table 1 : Calibration with Aqualytic reagents

Photometer used	Spectrophotometer		
Potassium iodate	EN ISO 7393-2	Aqualytic, free chlorine	Aqualytic, total chlorine
mg/l	Extinction		
0.00	0.000	0.004	0.007
0.025	0.006	0.010	0.012
0.05	0.012	0.016	0.020
0.10	0.025	0.032	0.034
0.15	0.039	0.046	0.051
0.20	0.050	0.061	0.066
0.25	0.063	0.077	0.079
0.30	0.076	0.091	0.095
0.35	0.089	0.105	0.109
0.40	0.101	0.117	0.124
0.45	0.115	0.133	0.137
0.50	0.127	0.151	0.152
0.75	0.187	0.219	0.226
1.00	0.246	0.287	0.301
1.25	0.302	0.367	0.366
1.50	0.359	0.429	0.435
1.75	-	0.497	0.490
2.00	0.452	0.548	0.564

Quadratic Regression			
n (c)	-0.020	-0.014	-0.014
m (b)	0.268	0.305	0.306
b (a)	-0.002	0.001	0.004
Sy	0.001	0.004	0.003
Sxo	0.006	0.012	0.010
Vxo (%)	1.1	2.0	1.6

Linear Regression			
Intercept	0.006	0.006	0.010
Slope	0.232	0.279	0.280
Sy	0.007	0.006	0.005
Sxo	0.029	0.021	0.019
Vxo (%)	5.3	3.3	3.0

Significant best fit	quadratic	quadratic	quadratic
----------------------	-----------	-----------	-----------

INSTITUT FRESENIUS

Limits of detection & quantitation (calculated from concentrations of up to 0.4 mg/l)			
Detection	0.007	0.01	0.01
Quantitation	0.023	0.04	0.04
VB (lower limit)	0.02	0.03	0.03
VB (upper limit)	0.04	0.08	0.07

I.2 Measurement results obtained with Hach reagents and their statistical evaluation

Table 2 : Calibration with Hach reagents

Photometer used	Spectrophotometer	
	Hach, free chlorine	Hach, total chlorine
mg/l	Extinction	
0.00	0.001	0.003
0.025	0.006	0.010
0.05	0.014	0.016
0.10	0.029	0.032
0.15	0.044	0.049
0.20	0.059	0.064
0.25	0.074	0.079
0.30	0.090	0.094
0.35	0.105	0.109
0.40	0.119	0.124
0.45	0.131	0.140
0.50	0.147	0.153
0.75	0.219	0.231
1.00	0.292	0.300
1.25	0.360	0.372
1.50	0.424	0.440
1.75	0.496	0.508
2.00	0.554	0.578

Quadratic Regression		
n (c)	-0.013	-0.011
m (b)	0.304	0.310
b (a)	-0.0010	0.0021
Sy	0.002	0.001
Sxo	0.006	0.004
Vxo (%)	1.0	0.7

Linear Regression		
--------------------------	--	--

INSTITUT FRESENIUS

Intercept	0.004	0.007
Slope	0.281	0.289
Sy	0.004	0.0039
Sxo	0.016	0.014
V _{xo} (%)	2.6	2.2

significant best fit	quadratic	quadratic
----------------------	-----------	-----------

Limits of detection & quantitation (calculated from concentrations of up to 0.4 mg/l)		
Detection	0.01	0.01
Quantitation	0.03	0.03
VB (lower limit)	0.02	0.02
VB (upper limit)	0.05	0.05

Evaluation

1. Regression :

During all calibrations, the quadratic regression provided the significant best fit.



The spread of figures around the calculated curves (quadratic regression) is described by the standard deviations V_{x0} associated with the procedure [3]. These are low and lie between 0.7% and 2.0%.

2. Limits of detection and quantitation :

The limits of detection and quantitation were calculated in accordance with DIN 32645: 1994 [2]. Only measured values as far as 0.40 mg/l were taken for calculation purposes, in order to ensure linearity and variance homogeneity. The quantitation limit (LOQ) is between 0.023 mg/l and 0.04 mg/l. No significant differences were observed between the data provided in EN ISO 7393 and figures obtained for the two powder reagents, since confidence intervals is overlap.

I.3 Graphical presentation of results : comparison of Aqualytic and Hach reagents

The following graphs show the results of measurements obtained by spectrophotometer for free chlorine and for total chlorine.

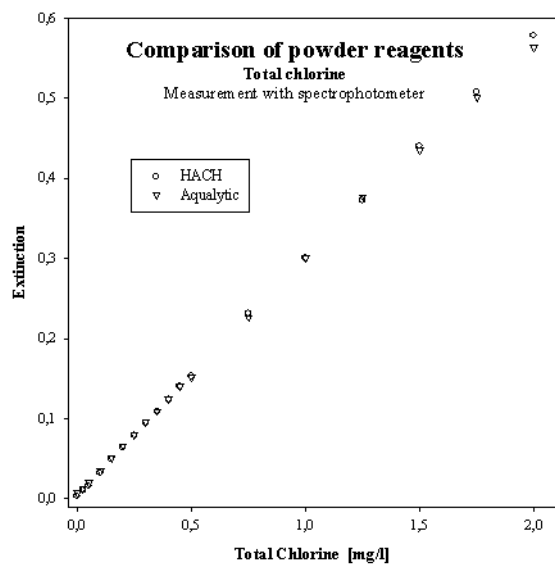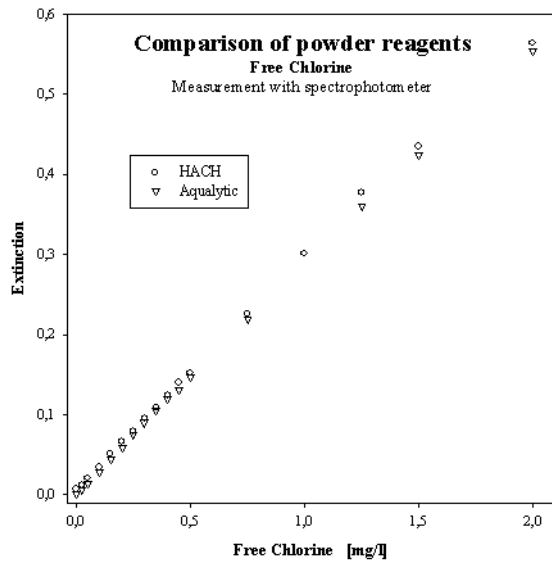

II Precision Measurements

Table 3 : Mean value t test (powder reagents for free chlorine)
Measurement using a spectrophotometer

Reagent	EN ISO 7393-2	Aqualytic	Hach	Aqualytic	Hach	Aqualytic	Hach	EN ISO 7393-2	Aqualytic	Hach
Concentr.	0.25 mg/l			1.00 mg/l		2.00 mg/l		1.50 mg/l		
	0.063	0.071	0.072	0.288	0.294	0.560	0.565	0.354	0.439	0.435
	0.064	0.071	0.075	0.288	0.291	0.561	0.560	0.358	0.437	0.432
	0.064	0.074	0.074	0.288	0.296	0.565	0.571	0.357	0.435	0.432
	0.064	0.073	0.074					0.357	0.434	0.432
	0.064	0.073	0.074					0.355	0.433	0.429
	0.063	0.073	0.075					0.354	0.436	0.432
	0.064	0.071	0.074					0.354	0.432	0.429
	0.063	0.071	0.073					0.353	0.432	0.429
	0.064	0.071	0.073					0.356	0.433	0.432
	0.063	0.071	0.073					0.358	0.433	0.435
Mean	0.064	0.072	0.074	0.288	0.294	0.562	0.565	0.356	0.434	0.432
Std. dev.	0.0005	0.0012	0.0009	0.0000	0.0025	0.0026	0.0055	0.0018	0.0023	0.0023
CV. %	0.81	1.67	1.29	0.00	0.86	0.47	0.97	0.52	0.53	0.52
Variance* 10 ⁻⁷	0.3	1.4	0.9	0	6,3	7,0	30	3,4	5,4	5,1
Number	10	10	10	3	3	3	3	10	10	10

Variance F Test					
<i>F</i> (EN-Lov.) assessment	5.37				1.59
	Significant difference				No sign. difference
<i>F</i> (EN-Hach) assessment			3.37		1.48
	No sig.		difference		No sig. difference
<i>F</i> (Lov.-Hach) assessment			1.59		1.08
			No sign. difference		No sign. difference
<i>F</i> (99%;1,f2)	5.35				5.35

Mean value t Test					
<i>PG</i>	3.73		3.90		0.95
<i>T</i> (99%)	2.88		4.60		4.60
assessment	Significant difference		No sign. difference		No sign. difference
					No sign. difference

Assessment of the Variance F Test

The results of the precision measurements were used to check whether there was any comparison between the distribution, or "scatter" of measured values for extinction via the F test. In each case, the values obtained using the method described in EN ISO 7393 were compared with the values obtained by Aqualytic and Hach methods. The F test was not carried out for concentrations of 1 mg/l and 2 mg/l, because the number of measurements (three in each case) was too small and the test would therefore be too insensitive.

The variation coefficients for all three procedures were extremely low, between 0.81% and 1.67% for the 0.25 mg/l standard, or between 0.52% and 0.53% for the 1.50 mg/l standard. No statistically significant differences between the different methods were noted for any of the comparisons for the 1.50 mg/l standard, or for two of the three comparisons for the 0.25 mg/l standard. Only for one of the comparisons using 0.25 mg/l was there a significant difference in distribution or "scatter" between EN ISO 7393 and Aqualytic methods. However, the difference was extremely small ($F = 5.37$; test figure = 5.35). The variation coefficient (CV) using the EN ISO 7393 method was 0.81%. The figure for the Hach method was 1.29%, with 1.67% for the Aqualytic method. These slight differences are of no practical significance¹.

Assessment of the mean value t test :

The results of extinction measurements according to EN ISO 7393 cannot be compared with those from Aqualytic or Hach, because other concentration conditions apply which must result in different extinctions.

A statistically significant difference was noted between the mean extinction figures for Aqualytic and Hach for the samples having a concentration of 0.25 mg/l of free chlorine. However, the difference is very small (Aqualytic = 0.072; Hach = 0.074) and therefore of no practical significance. No statistically significant differences were noted at any of the other concentrations.

¹ This becomes also apparent if the level of measurement accuracy is calculated from the measured distribution : EN ISO 7393 (0.25 ± 0.004); Hach (0.25 ± 0.006) and Aqualytic (0.25 ± 0.008) mg/l (VB 95% or $k = 2$).

III Calibration with potassium permanganate

III.1 Comparison of calibrations with potassium iodate and potassium permanganate in line with EN ISO 7393-2: 2000

Measurements with potassium iodate were carried out in accordance with EN ISO 7393-2: 2000. Thereafter, appropriate standards were used with potassium permanganate. The results are shown in Table 4 :


Table 4 : Results of measurements with potassium iodate and potassium permanganate in line with EN ISO 7393-2: 2000

Standard mg/l	KIO ₃	KMnO ₄
0,00	0,001	0,001
0,10	0,024	0,024
0,25	0,062	0,061
0,50	0,124	0,124
1,00	0,243	0,240
1,50	0,350	0,346

Assessment :

The regression calculation results in an intercept of 0.0003 and a slope of 0.988. If the measured extinctions were fully in line, the figures would be 0 and 1. The calibrations with potassium iodate and with potassium permanganate are thus similar for all practical purposes.

Results in graphical form

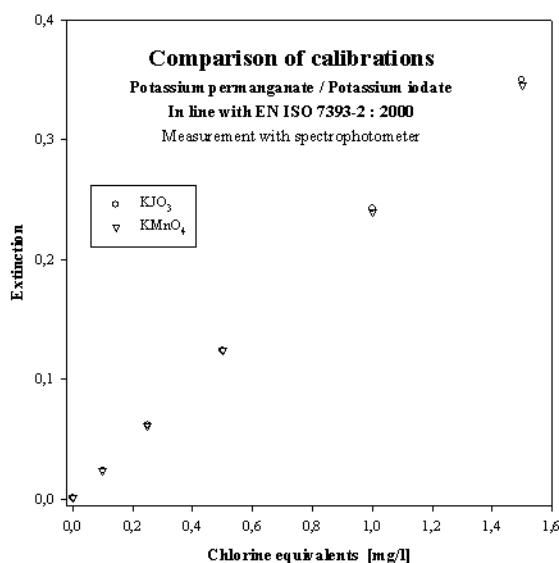


III.2 Comparison of calibrations with potassium permanganate, using reagents for free chlorine from Aqualytic and from Hach.

Extinctions for free chlorine were determined, using potassium permanganate standards.

Table 5 : Calibration with potassium permanganate

Standard KMnO ₄ mg/l	Free Chlorine	
	Aqualytic	Hach
0.00	0.001	0.001
0.10	0.027	0.026
0.25	0.070	0.073
1.00	0.290	0.290
1.50	0.420	0.415

Results in graph form :

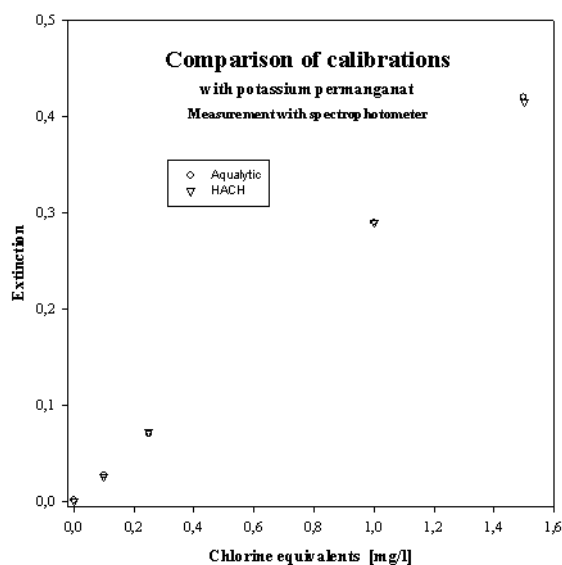

Assessment :

The regression calculation results in an intercept of 0.0011 and a slope of 0.990. If the measured extinctions were fully in line, the figures would be 0 and 1. For all practical purposes, therefore, the calibrations with potassium permanganate are similar for both powder reagents.

Bibliography :

- [1] EN ISO 7393-2 : 2000 : "Determination of Free Chlorine and Total Chlorine"; 2000-04
Determination-chlorine

- [2] DIN 32 645 : "Demonstration, Logging & Determination Limits"; May 1986
- [3] E DIN 38402-71 : "Equivalence of two Analysis Procedures, based on a Comparison of Analysis results and their Statistical Evaluation; Procedure for Quantitative Characteristics with a Continuous Value Spectrum (A 71)"; 2001-10

INSTITUT FRESENIUS AG



Dr. Wolfgang Adolph



Dr. Udo Krischke

Appendix

Measurements with a Hach photometer, to check the inter-changeability of Aqualytic and Hach reagents

Assessment :

In practice, both powder reagents tested produced comparable results when used with the Hach photometer. With totally compliant results, the measurement points would lie exactly on the dashed line.

Results in graphical form :

